

# Anaplasma Ab / Ehrlichia Ab Test Kit

## Principles

**Anaplasma Ab test Kit:** SensPERT™ Anaplasma Ab Test Kit is designed to detect the antibodies of anaplasma in canine whole blood, serum or plasma. After being absorbed into the cellulose pad, the antibodies of anaplasma move and bind with gold-colloid complex of canine antigen of the conjugate pad, forming Ag-Ab complex. This complex, then, forms Ag-Ab-Ag direct sandwich binding with antigen of anaplasma in the nitrocellulose membrane. The test results can appear on Control (C) and Test (T) lines where the principles of immunochromatography are used.

**Ehrlichia Ab Test Kit :** SensPERT Ehrlichia Ab Test Kit is designed to detect Ehrlichia canis antibodies in whole blood, serum or plasma. After being absorbed into the cellulose pad, the antibodies of Ehrlichia canis move and bind with gold-colloid complex of Ehrlichia canis antigen of the conjugate pad, forming Ag-Ab complex. This complex, then, forms Ag-Ab-Ag direct sandwich binding with p30/p30-1 antigen (Ag) of Ehrlichia canis in the nitrocellulose membrane. The test results can appearance on Control and Test lines where the principles of immunochromatography are used.

## Characteristics

- 1) One-step rapid test of Anaplasma Ab / Ehrlichia Ab
- 2) Rapid test results between 5 ~ 10 minutes
- 3) Expensive equipment not required
- 4) Easy storage and maintenance
- 5) High-purity and high-quality materials of the test kit increase its sensitivity and specificity.

## Materials (10 tests/kit)

- 1) Test ----- 10 units
- 2) Diluent (buffer) ----- 3 ml x 1 unit
- 3) Disposable dropper for sample collection ----- 10 units

## Composition

Specimen well (S: for dropping), Test line (T), and Control line (C) are marked on the device. Inside of it, the strip is composed of sample pad, conjugate pad, nitrocellulose membrane (test paper) and absorbent pad

## Effect

Detection of Anaplasma antibody and Ehrlichia antibody from canine whole blood, serum, or plasma

## Uses

- 1) Specimen  
Canine Whole blood, serum or plasma
- 2) Test procedure
  - a) When specimen and test kits are stored at cold circumstances (2-8 °C), put them at room temperature for 15 ~ 30 minutes before use.
  - b) Take out a device from a pouch and place it on a horizontal surface.
  - c) Using a dropper as a pipette, obtain the specimen and dispense 1 drop ( 10  $\mu\text{l}$  ) of the fluid into the specimen well (S).
  - d) When the specimen is completely absorbed into the specimen well (S), add 2 drops ( 80  $\mu\text{l}$  ) of buffer.
  - e) Read the test results between 5 ~ 10 minutes.

### ◆ Invalid result after 10 minutes

- 1) Interpretation of the results  
A purple band should appear on the control line regardless of the test result. The presence of another band on the test line determines the result.

**Control Line (C):** The line should always appear. If this line does not appear, the test should be considered invalid. This might be because of impure buffer or the lack of specimen. It should be tested again with another kit.

**Test Line (T):** The presence of Anaplasma Ab and/or E. canis Ab determines the test line.

### (1) Anaplasma / E. canis Negative



### (2) Anaplasma Positive / E. canis Negative



### (3) Anaplasma Negative / E. canis Positive



### (4) Anaplasma / E. canis Positive



### (5) Retesting

- a) Both Test and Control lines do not appear.



- b) Test line only appears.



## Further examinations

This test is for primary screening only. Consult veterinarians for further necessary examinations to obtain clinical test results.

## Precautions

- 1) Use for canine *in-vitro* diagnostic purposes only.
- 2) Use within 10 minutes after opening the pouch because the test kit is very sensitive to moisture and its effect may diminish.
- 3) Be careful of not touching the result window.
- 4) Every specimen should be used with different droppers.
- 5) For testing, the buffer included should be used.
- 6) Do not use specimen being contaminated with microbes, which may cause false positive or false negative result.
- 7) Deal with specimen carefully. They can deliver unknown virus or infectious bacteria.
- 8) Use disposable gloves when you suspect the infection caused by specimen. And wash your hands later.
- 9) Dispose solid wastes after sterilizing them at 121 °C for over 1 hour.
- 10) Do not use the kit when its pouch is torn, sealing is not good in shape or expiration date is passed.

## Storage method

The test kits stored at 2-30°C can be used for 24 months after manufacturing. Do not keep them in a refrigerator. However, if they are stored under cold circumstances, keep them at room temperature for 15 ~ 30 minutes before use.

## Exchange

The test kits are manufactured under strict quality control system. Nevertheless, if they are deteriorated during delivery, ask our distributors for exchange.

## Liability

The entire risk due to the performance of this product is assumed by the purchaser. The manufacturer shall not be liable for indirect, special or consequential damages of any kind resulting from use of this product.

Date issued : Sep. 09. 2013  
AI24-12E-01


# Instruction for Anaplasma Ab / Ehrlichia Ab test



Sample fill line (black line) : 1 drop ( 10  $\mu$ l )

# 1


Sampling  
& loading

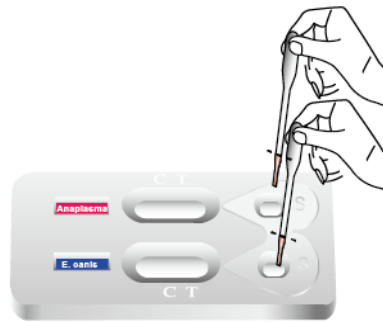

1 drop of sample  
•• Do not overload the sample!!

# 2

Absorption

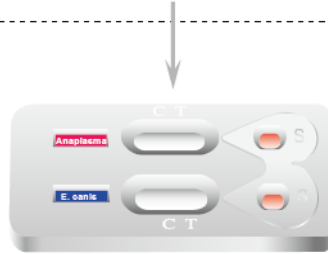

Wait for complete absorption


# 3

Buffer addition

00:00:00



2 drops of buffer  
•• after complete absorption

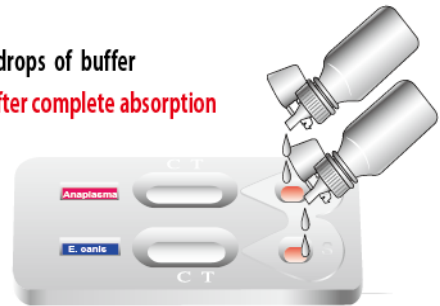

# 4

Reading

00:05:00~00:10:00




+



Read the result between 5 ~ 10 min

-

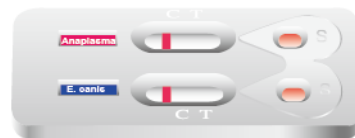

# 5

Discard

00:10:00



Discard the used device  
In valid result after 10 min

